



iQ-Flatlight

User Manual

June 21, 2023





CONTENT

1	INTRODUCTION	3
1.1	Conformity	3
1.2	Intended use	3
1.2.1	Departing from described setup	3
1.2.2	USB connection	3
1.3	General safety information	4
2	GETTING STARTED.....	4
2.1	Scope of delivery	4
2.2	Set-up homogeneity	4
2.2.1	Height setting	5
2.2.2	Setup around chart	6
2.3	Setting up the devices in the iQ-LED software and creating illuminants.....	7
2.4	Low light scenes	10
3	OPERATING INSTRUCTIONS HARDWARE.....	10
3.1	Overview display and ports	10
3.2	Connecting the hardware	12
4	OPERATING INSTRUCTIONS SOFTWARE	13
4.1	Requirements.....	13
4.2	Software installation.....	13
4.3	Starting the system.....	13
4.3.1	Spectrometer settings.....	13
4.3.2	Spectrometer calibration	13
4.3.3	iQ-LED calibration	13
4.3.4	Calibration device handling.....	14
4.4	Low-intensity use	14
5	ADDITIONAL INFORMATION	15
5.1	Maintenance.....	15
5.2	Spectrometer removal for calibration	15
5.3	Care instructions	17
5.4	Disposal Instructions	17
6	TECHNICAL DATASHEET	17

1 INTRODUCTION

Important information: Read the manual carefully before using this device.

Inappropriate utilization may cause damage to the device, to the DUT (device under test), and/or other components of your setup.

Please keep these instructions in a safe place and pass them on to any future user.

1.1 Conformity

We, Image Engineering GmbH & Co. KG, hereby declare that the "iQ-Flatlight" corresponds to the essential requirements of the following EC directive:



- Electromagnetic Compatibility - 2014/30/EU
- RoHS 2 - 2011/65/EU
- Low Voltage - 2014/35/EU

1.2 Intended use

The iQ-Flatlight is designed as a spectrally tunable source to illuminate large areas. It is based on iQ-LED technology, includes a micro-spectrometer, and is controlled with the iQ-LED control software.



- Only suitable for indoor use.
- Place your system in a dry, constantly tempered environment without interfering light.
- The optimal ambient temperature range is 22 to 26 degrees Celsius. The maximum ambient temperature range is 18 to 28 degree Celsius.
- The optimal system temperature range, displayed in the software user interface, is between 35 and 50 degrees Celsius. The system has internal temperature management, if there is an error regarding the internal temperature, you will get a warning message, and the system automatically turns off to avoid any damage.

1.2.1 Departing from described setup

The following steps must be performed in the correct chronology to allow frictionless commissioning. Departing from the chronology may lead to an incorrect working device.

1. Install the iQ-LED software
2. Connect iQ-Flatlight to power and via USB to the PC
3. Switch iQ-Flatlight on; the system drivers will be installed
4. After drivers are installed, restart the software

1.2.2 USB connection

Only an appropriate USB connection allows the error-free operation of iQ-Flatlight. Use delivered USB cables. If you need to extend the USB connection to longer distances, please check if powered hubs/repeaters are necessary.

1.3 General safety information



WARNING!

Some LEDs emit invisible light in the IR and the near UV area.



- **Do not** look directly into the emitted light or through the optical LED system.
- **Do not** look directly at the open sphere or light source when using high intensities or sequences with low response time.
- **Do not** open the device without instructions from the Image Engineering support team or when connected to the power supply.

2 GETTING STARTED

2.1 Scope of delivery

- Two iQ-Flatlight, each with a spectrometer (calibration device) and Rolling Cart
- 2 x power cords
- 2 x USB cables
- Control software
- Calibration protocol

Optional equipment:

- **iQ-Trigger:** The iQ-Trigger is a mechanical finger that can press the release button within 25 ms. When working with touchscreens, exchange the solid fingertip for a touch pen tip.
- **Gossen Digipro F2:** An exposure meter for high-precision incident light measurement. Perfect for ensuring the illumination uniformity of reflective test charts.
- **PRC Krochmann Radiolux 111:** The Radiolux 111 is a high-precision instrument for photometric measurements.

2.2 Set-up homogeneity

To get uniform illumination on your test chart, you must find the optimal position of your iQ-Flatlights beside your chart.


2.2.1 Height setting

- Start with the height setting. The iQ-Flatlights should be centered at the chart level. (see image below)



We recommend changing the height setting using two people.

- The first person holds the iQ-Flatlight (see image 1).
- The second person loosens the screws on the right and left on the inner side of the iQ-Flatlight (see image 2).
- Loosen the screws of the center brace on the backside of the iQ-Flatlight to move it closer to the other brace (see image 3).
- The first person can push the iQ-Flatlight up or down.
- If you have the correct height, tighten the screws and
- Tighten the screws of the brace.

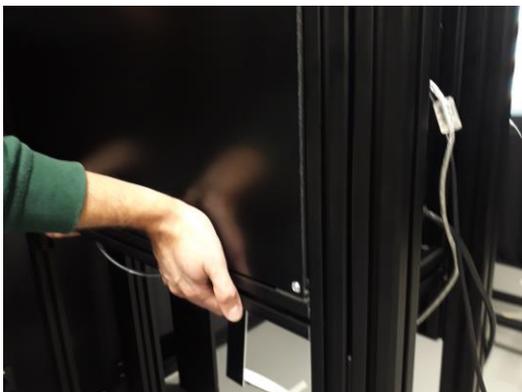

Hold iQ-Flatlight (image 1)



Second person loosens the screw (image 2)



Loosen the screws of the center brace on the backside of the iQ-Flatlight (image 3).

2.2.2 Setup around chart

Start by placing your iQ-Flatlights as close as possible to your chart (~150 cm distance from the chart center to the iQ-Flatlight) at an angle of 45 degrees, depending on your camera's optical axis. From there, begin measuring the uniformity of illumination on your test chart and adjust the position of your flatlights to suit your test setup best. We recommend using an exposure meter (see 2.1 optional equipment) to check the uniformity of the light. Measure all four corners and the center of the chart. The values shouldn't deviate 1/10 f-stop from each other.



2.3 Setting up the devices in the iQ-LED software and creating illuminants

Complete the following procedure for each iQ-Flatlight with a luxmeter (see 2.1 optional equipment).



- Ensure room lighting and fluorescent tubes in the iQ-Flatlights are switched off.
- If necessary, detach the red protection from the spectrometer's measuring head.
- Open the iQ-LED software:
 - (1) open the device manager by clicking the gear wheel on the top left
 - (2) add a new device by clicking the (+)
 - (3) name the device comprehensibly
 - (4) chose if necessary, a suitable icon
 - (5) & (6) drag and drop the LED device and the spectrometer from "Unassigned Components" to "Target Components"
 - (7) close "managing devices"



- Pull up the calibration device into the measuring position.



- Open the spectrometer settings by clicking the (1) gear wheel near the icon the in the iQ-LED software, perform the auto detection (2) and a dark measurement (3), then turn on the calibration light (4) for the software to calculate the compensation factor.
- Pull down the calibration device into the standby position.

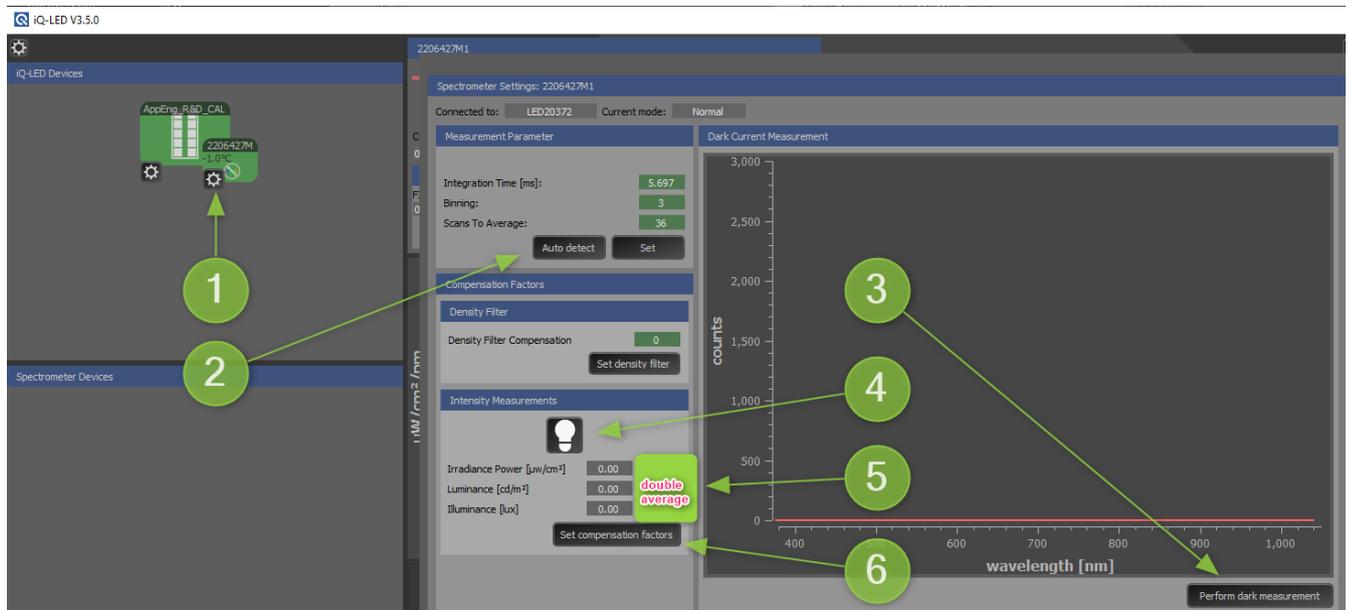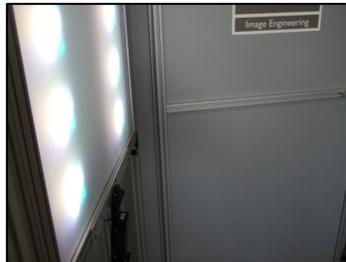

- Measure the four corners and the center of the chart with a luxmeter (it will be inhomogeneous with only one iQ-Flatlight switched on) and calculate the average value. Double this value and insert it (5) at the corresponding (in general, you measure lux) spot into the software.
- Set (6) the compensation factor.
- Then close the window with the spectrometer settings.

- Pull up the calibration device into the measuring position.



- Open the iQ-LED Setting by clicking the gear wheel underneath the icon (1) and let the software perform a new spectral calibration (2). If this device already has an existing calibration, please only renew that one (3). There is no need to store outdated calibration settings.
- Close this window.

iQ-LED V3.5.0

2206427M1

Color values

Illuminance [lx]	X	0.00	0.7
	Y	100.00	0.6
	Z	0.00	0.5
CCT [K]	x	0.0000	0.4
	y	0.0000	0.3

Chromacity map

iQ-LED Settings: LED20372

Device-Information

LED20372

Advanced settings

Standard Modules

Module ID	8
Temperature [°C]	20

Extension Modules

Trigger

Trigger duration 100 ms

Start Warm Up

Device calibration (Please warmup device before calibration)

Mo Okt 24 11:21:12 2022

All channels

- Channel 409nm
- Channel 423nm
- Channel 442nm
- Channel 461nm
- Channel 480nm
- Channel 505nm
- Channel 541nm
- Channel 579nm
- Channel 598nm
- Channel 617nm
- Channel 636nm
- Channel 644nm
- Channel 660nm
- Channel 680nm
- Channel 703nm
- Channel 728nm
- Channel 745nm
- Channel 767nm
- Channel 782nm
- Channel 808nm

μW/cm² /nm


wavelength [nm]

Close

AppEng_RD_CAL



- Generate an illuminant. Choose the spectral distribution (1) by its name from the list. Determine the desired intensity in lux (2). Note that the "i" button (3) calculates the maximum possible intensity of the chosen spectrum. When the illuminant is done being created, store it via drag and drop (4) on the computer.

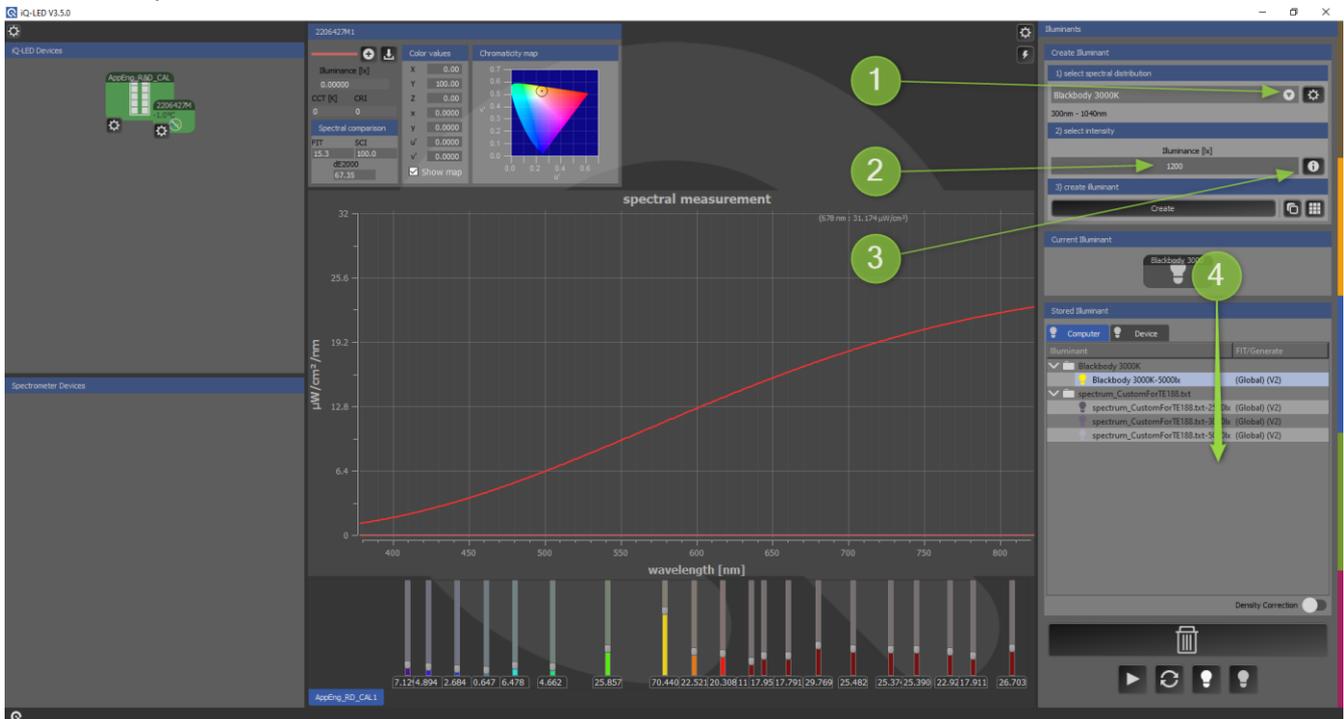

- Unplug the iQ-Flatlight and plug in the second one. Proceed the same way as with the first one.
- Equal illuminants with the same name will appear in the list when you activate both iQ-Flatlights by clicking the (+) at the iQ-LED icon in the left part of the GUI. Those will be activated simultaneously in both light sources.

2.4 Low light scenes


You can generate low-light illuminants by switching off single modules. According to the specification, you can generate down to 25lx with standard daylight illuminants. By switching off nine of ten modules, you can theoretically generate 2.5lx.

Another way to create low-light illuminants (e.g., VCX) is to use ND filters. Please get in touch with our application engineers in the customer support department for more details. Suitable suppliers are, for example, Lee or Rosco, among others.

3 OPERATING INSTRUCTIONS HARDWARE

3.1 Overview display and ports

- 1 x USB port for software control
- 1 x port for the power adapter
- 1 x trigger output

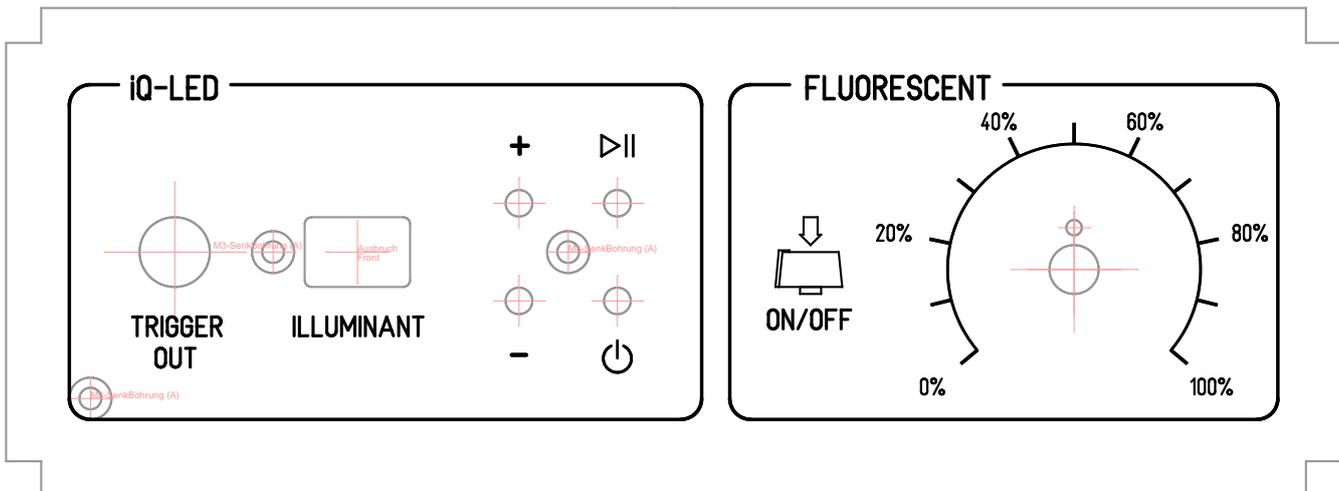

Use the control panel to set different light settings for the iQ-LEDs and the fluorescent tubes:


iQ-LED:

- With the "+" and "-" buttons, you can switch between 44 saved illuminants.
- Numerical display to show the storage of the illuminants.
- With the play and stop button, you can start and stop a saved light sequence with different illuminants (it is possible to save one sequence on the device).
- With the power button, you can turn on and off the light.
- There are three pre-stored illuminants on your device (the intensity of each illuminant is shown in the acceptance protocol of your device):

- 1: illuminant A (default illuminant)
- 2: illuminant D50
- 3: illuminant D75

Fluorescent (only for iQ-Flatlight with Fluorescent Tubes):

- When pressing the rotary knob, you can turn on or off the fluorescent tubes.
- While turning the rotary knob, you can set the intensity from low (0%) to high (100%).
- Note: To store your generated illuminants or sequences on your device, please follow the iQ-LED Software user manual instructions.

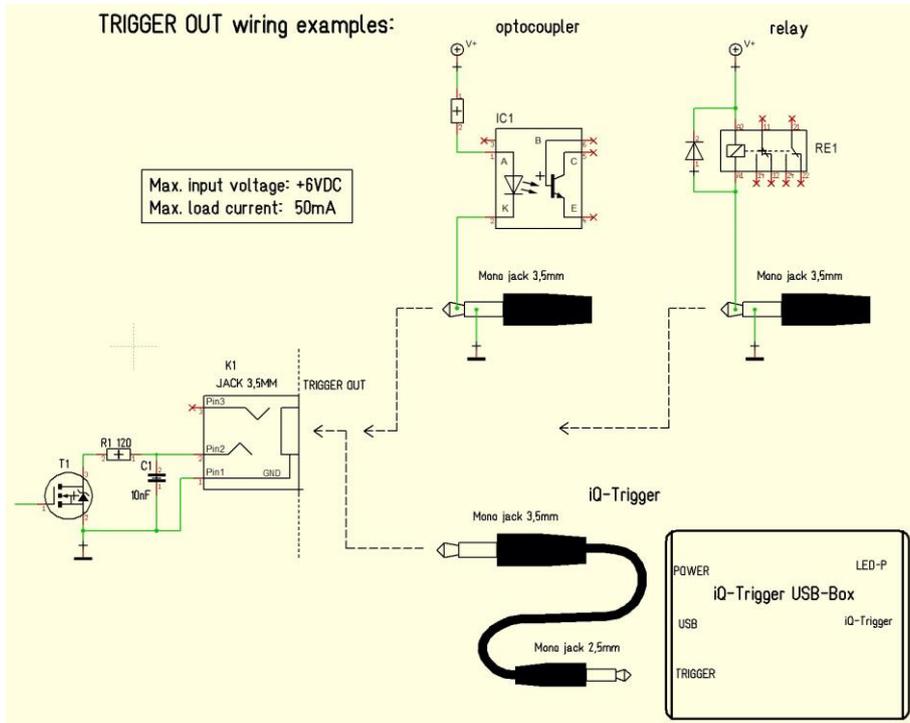

The default duration value for the trigger output is 500 ms. This value can be modified with the iQ-LED API. A signal is sent out to the trigger output while changing the illuminates or the intensity of LED channels. For example, it can synchronize your test setup with an iQ-Trigger (See 2.1 optional equipment).

3.2 Connecting the hardware

Connect the power cord to the power outlet on the side of your iQ-Flatlight. Connect the USB cable from the Flatlight to your PC and turn on the Flatlight (the power switch is next to the power outlet). Then connect the USB cable from the spectrometer calibration device to your Flatlight. The system will install the spectrometer and iQ-LED driver on your PC (this will take a few seconds). You can check the installation in your hardware manager:



Hardware Manager: active iQ-LED devices and spectrometer



4 OPERATING INSTRUCTIONS SOFTWARE

4.1 Requirements

PC with Windows 7 (or higher) operating system
One free USB port

4.2 Software installation

Install the iQ-LED control software before connecting the hardware. Follow the setup instructions from the iQ-LED control software manual.

4.3 Starting the system

Start the iQ-LED software by clicking the 'iQ-LED.exe' or the iQ-LED icon on your desktop.

Follow the iQ-LED software manual to control your iQ-Flatlight.

NOTE

The iQ-LED devices can operate with high precision only when setup and calibration are performed correctly. Consult the iQ-LED software manual for a comprehensive description, and read it carefully.

4.3.1 Spectrometer settings

The iQ-LED software (see iQ-LED software manual) automatically generates the best spectrometer settings for your lighting conditions after pressing the "auto-detect" button. It is also possible to manually set the spectrometer settings for special applications. If you have further questions, please contact the Image Engineering support team.

4.3.2 Spectrometer calibration

Your spectrometer comes fully NIST traceable calibrated. We recommend recalibrating the spectrometer once a year, regardless of the operating hours. If a spectrometer calibration is required, please contact Image Engineering.

Note: Before removing the spectrometer, measure and note the lux value of a predefined standard illuminant.

4.3.3 iQ-LED calibration

The individual LED lights of the iQ-LEDs, inside the iQ-Flatlight, depend on many different types and wavelengths. Some LEDs will slightly change their intensity level and peak wavelength in the first 500-600 working hours because of a burn-in effect.

The LEDs will also degrade in intensity during their lifetime. To ensure that all measurements, including the auto-generated and standard illuminants, are correct, you must perform a spectral calibration regularly.

You must also consider the degradation of the LED when saving self-defined presets. Suppose you save a preset with LED channels that uses its maximum intensity. In that case, the possibility exists that this intensity cannot be reached after the burn-in time or the long-time degradation of the LED. In this case, you will get a warning message from the iQ-LED control software.

During the first 500-600 working hours, we recommend performing a spectral calibration every 50 operating hours.

After the first 500-600 operating hours, a calibration of every 150 working hours suffices.


Other factors that indicate the need for a spectral calibration include unsatisfactory illuminant generation, the aberration of the intensity values, or a spectral curve that does not fit the predefined standard illuminants of the corresponding preset.

- The spectrometer works correctly
- The spectrometer settings are correct
- All LED channels work correctly
- The dark measurement is correct
- Your measurement environment is correct
- Your ambient temperature is correct

How to perform the spectral calibration is described in the iQ-LED control software manual.

4.3.4 Calibration device handling

The calibration device must be in the 'standby position for normal usage.' If you want to calibrate your system, generate a new illuminant or set a new intensity, and then set the calibration device to the 'measure position' via the folding mechanism:

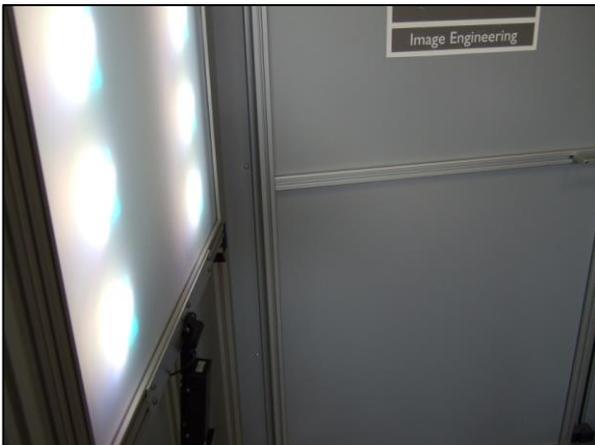

The calibration device is in the "standby position."



The calibration device is in the "measure position."

Please be careful with your spectrometer, the fiber, and the measuring reflector. Avoid any force effect or contamination of the device. If you have finished your light setting or calibration via the iQ-LED control software, you can push back the calibration device to the 'standby position.'

4.4 Low-intensity use

The spectral measurement values will fluctuate when using your system with very low intensity. The lower the intensity, the higher the fluctuation. The generated light is still stable up to a certain point. The noise of the internal spectrometer's spectral measurement causes the values' fluctuation. The lower the light intensity, the higher the noise influence. An approximate value will no longer be possible when using standard illuminants with an intensity lower than 25 lux.

5 ADDITIONAL INFORMATION

5.1 Maintenance

The spectrometer requires a recalibration once a year, regardless of the operating hours. You can still use the stored Illuminants on the iQ-Flatlight when the spectrometer is removed.

Please contact Image Engineering for shipping details before sending the spectrometers.

5.2 Spectrometer removal for calibration



**Do NOT remove the fiber from the spectrometer.
The spectrometer must be calibrated with the fiber.**

A spectrometer without the fiber or cap may be permanently damaged by dust.

- Unplug the USB cable and remove the cable ties.
- Unscrew the fiber from the calibration device (place a cap on the fiber tip).



- Ensure both the USB cable and the fiber are dangling loosely.
- Unscrew the plate holding the spectrometer using the knurled screws.
- Pack the spectrometer in a box while still on the holding plate.
- Put the spectrometer in the box it was shipped in if you still have it. Alternatively, use any other box; ensure the fiber is not bent too much.
- Use cushioning (e.g., bubble wrap) to protect the spectrometer from shock.





5.3 Care instructions

- Do not touch, scratch, or pollute the diffuser.
- If there is any dust on the diffuser, clean it with an air blower.
- Do not remove the fiber from the spectrometer. Otherwise, the calibration is invalid, and the spectrometer must be **recalibrated!**

5.4 Disposal Instructions

After the service life of the iQ-Flatlight, it must be disposed of properly. Electrical and electromechanical components are included in the iQ-Flatlight. Observe your national regulations and ensure that third parties cannot use the iQ-Flatlight after disposal.

Contact Image Engineering if assistance for disposal is required.

6 TECHNICAL DATASHEET

See the annex for the technical data sheet. It can also be downloaded from the website of Image Engineering: <https://image-engineering.de/support/downloads>.